


Flow Chart Specific for FSIS Laboratory Confirmation of Aminoglycosides by UHPLC-MS/MS

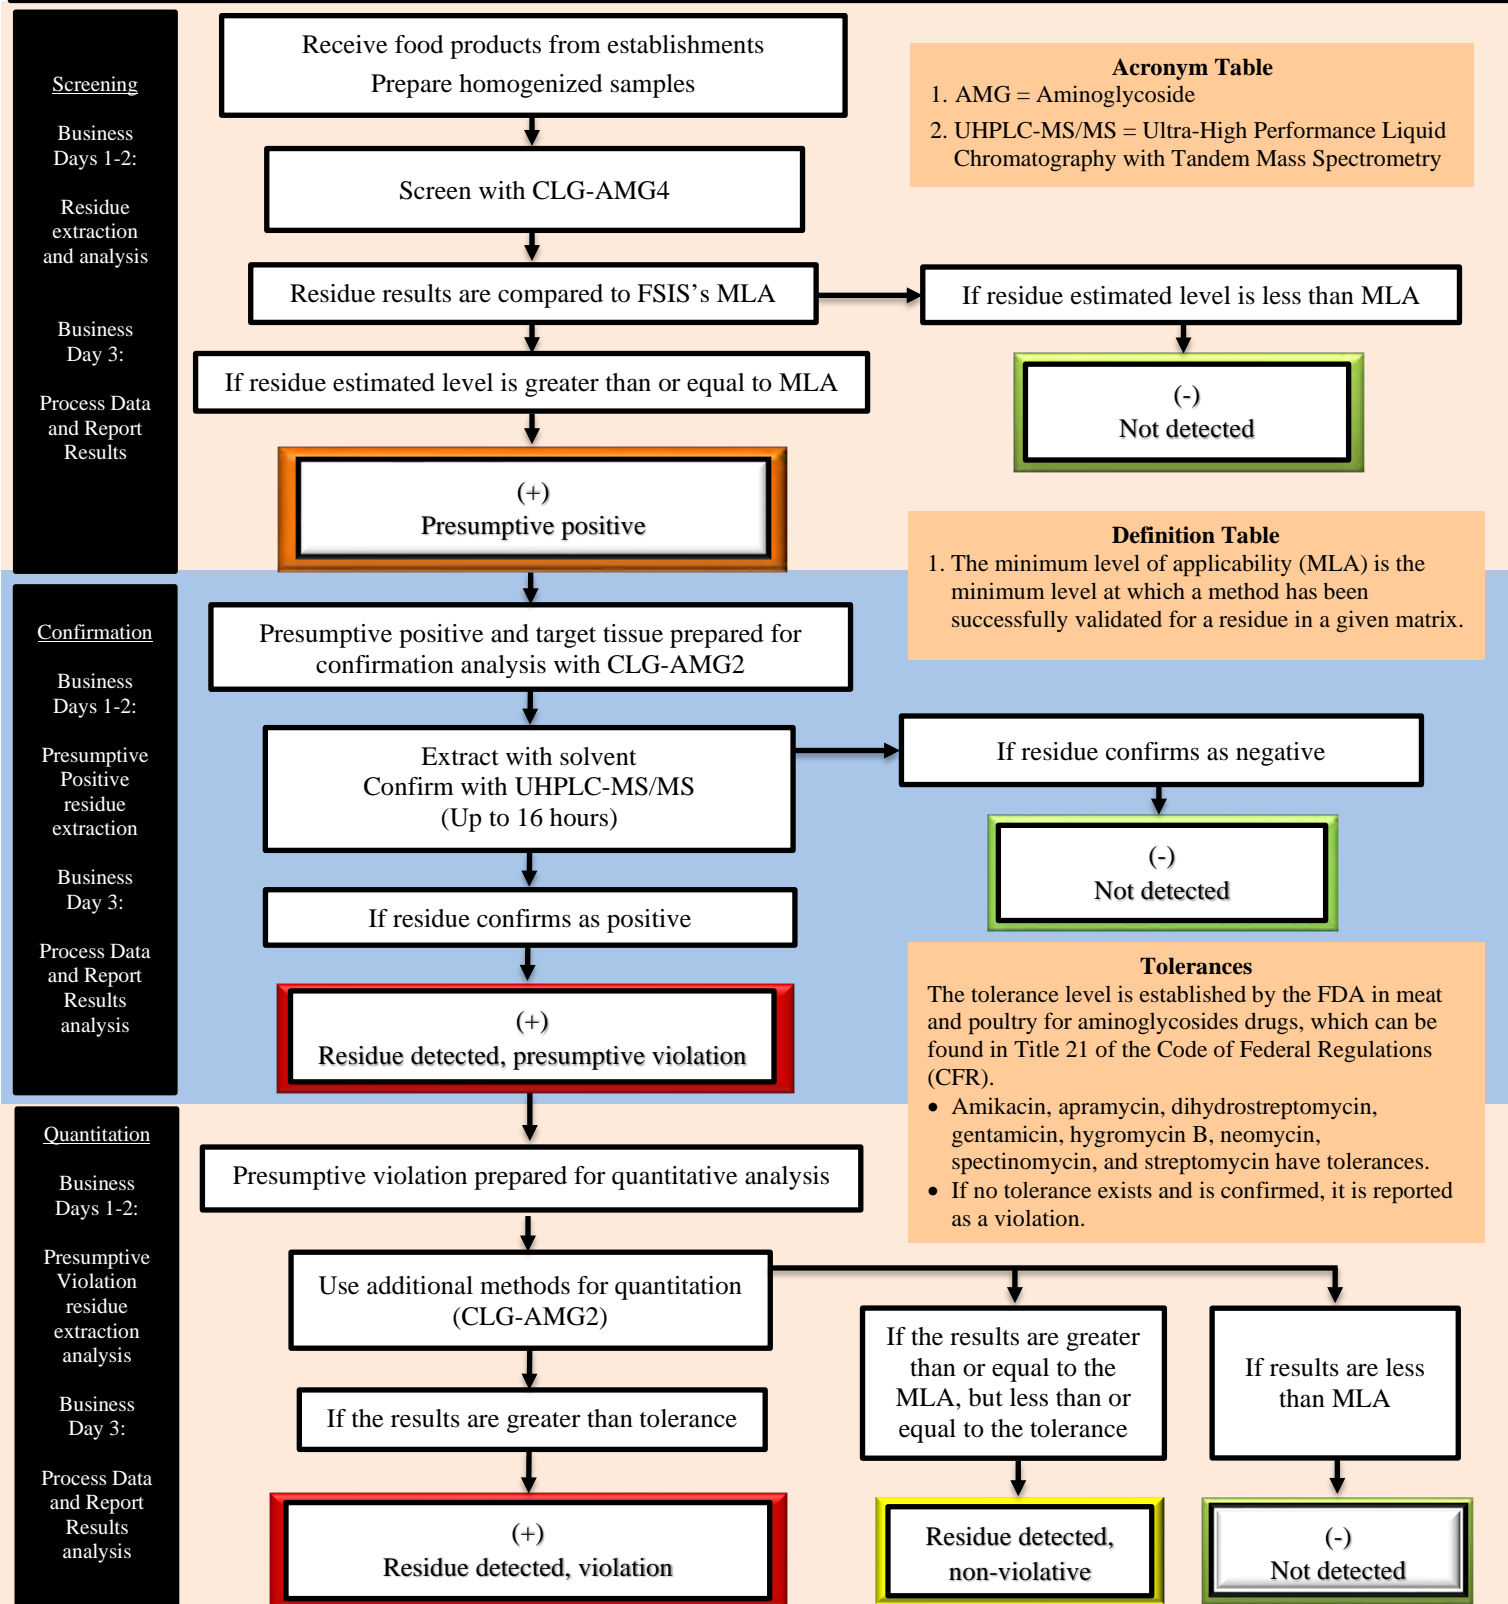

Blue background represents testing for the scope of CLG-AMG2. CLG-AMG4 and CLG-AMG2 are screening and confirmation methods, respectively, however, if quantitation is required, CLG-AMG2 will be used when necessary to quantitate the positive residue.

The Notice of Change for CLG-AMG2 Appendix 1.00 is found in CLG-AMG2.