


Flow Chart Specific for FSIS Laboratory Confirmation of Avermectins by UHPLC-MS/MS

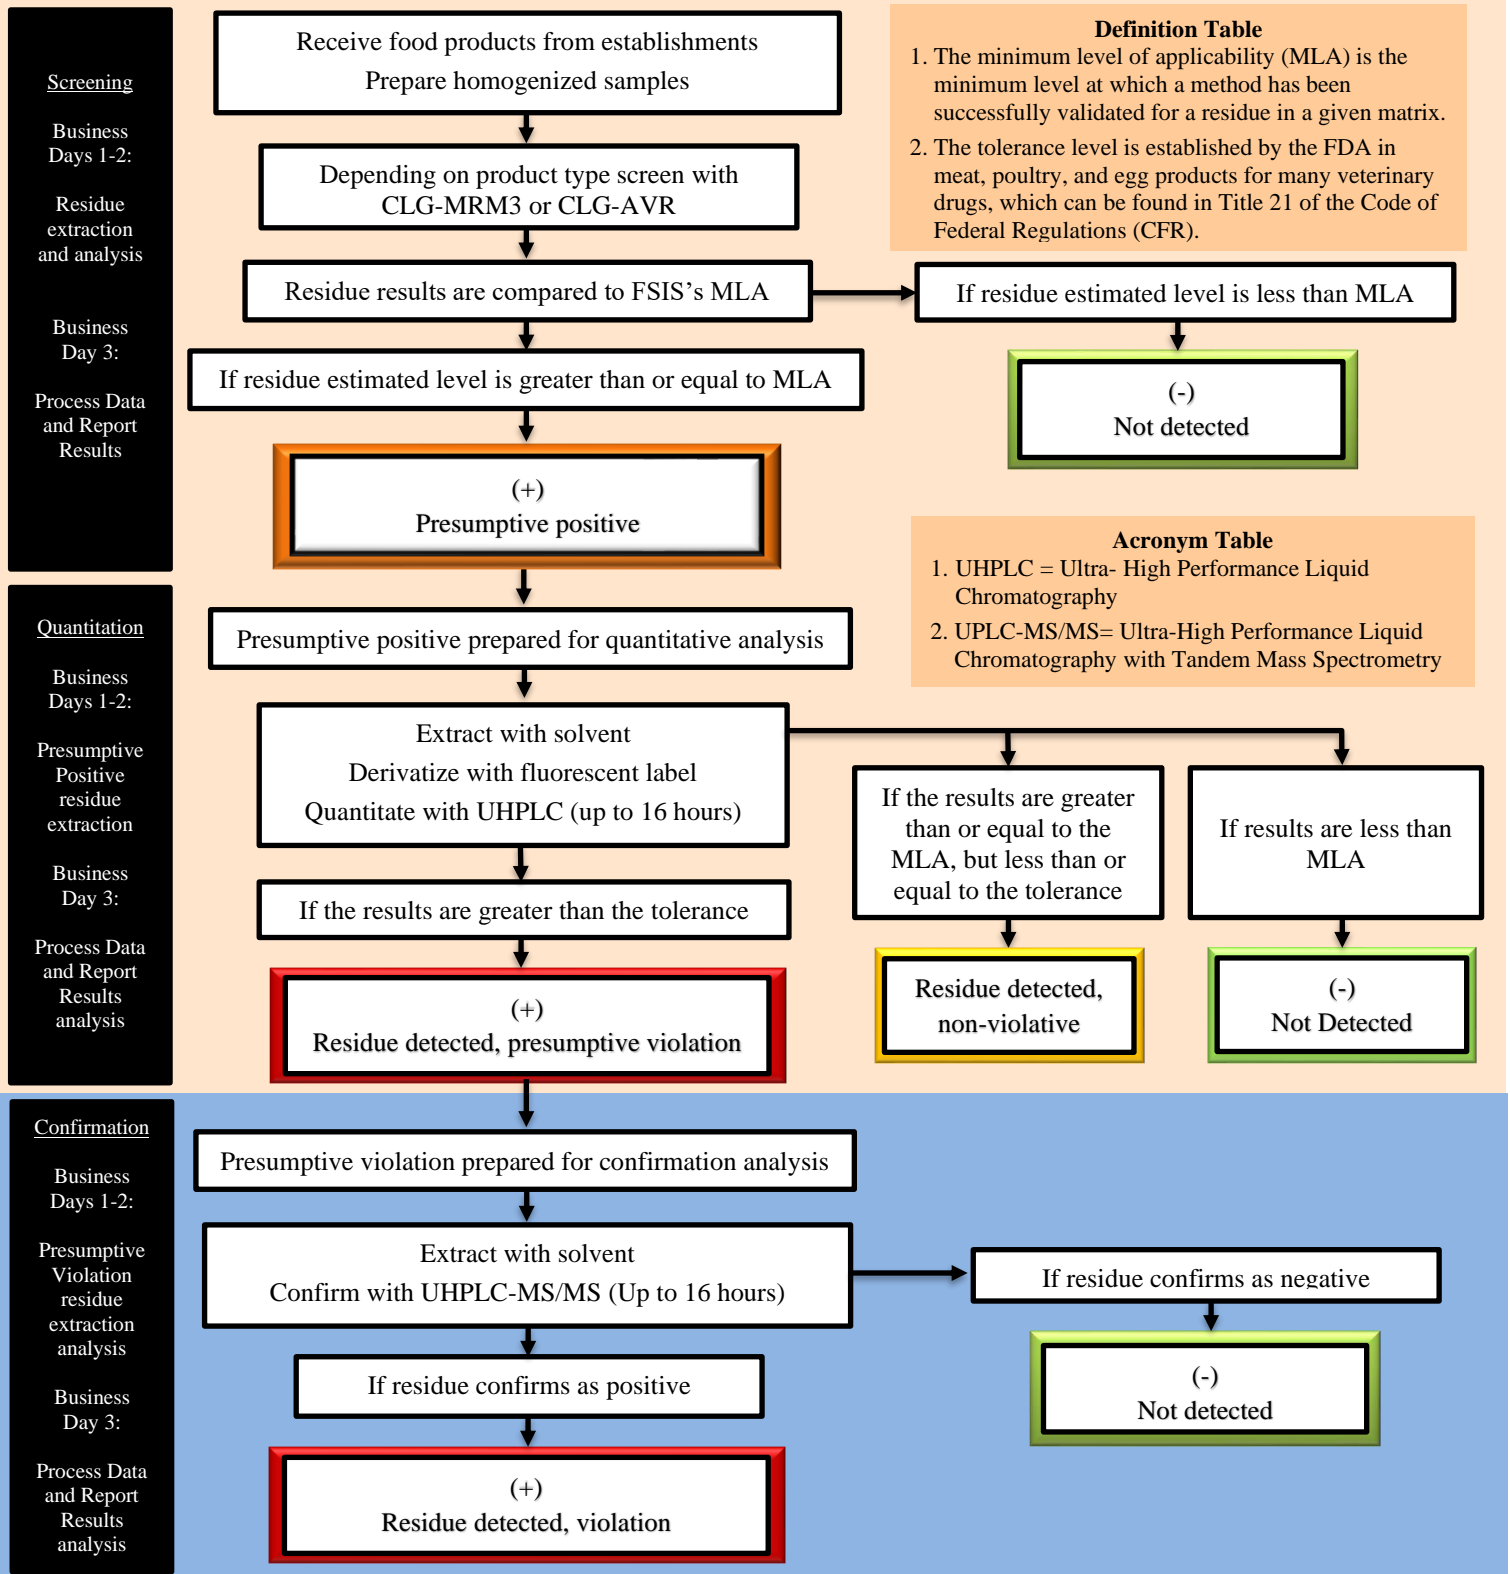

Blue background represents testing for the scope of CLG-AVR2

The Notice of Change for CLG-AVR2 Appendix 1.00 is found in CLG-AVR2.