


# Flow Chart Specific for FSIS Laboratory Multi-Residue Screening of Animal Drug Residues and Pesticides by UHPLC-MS/MS

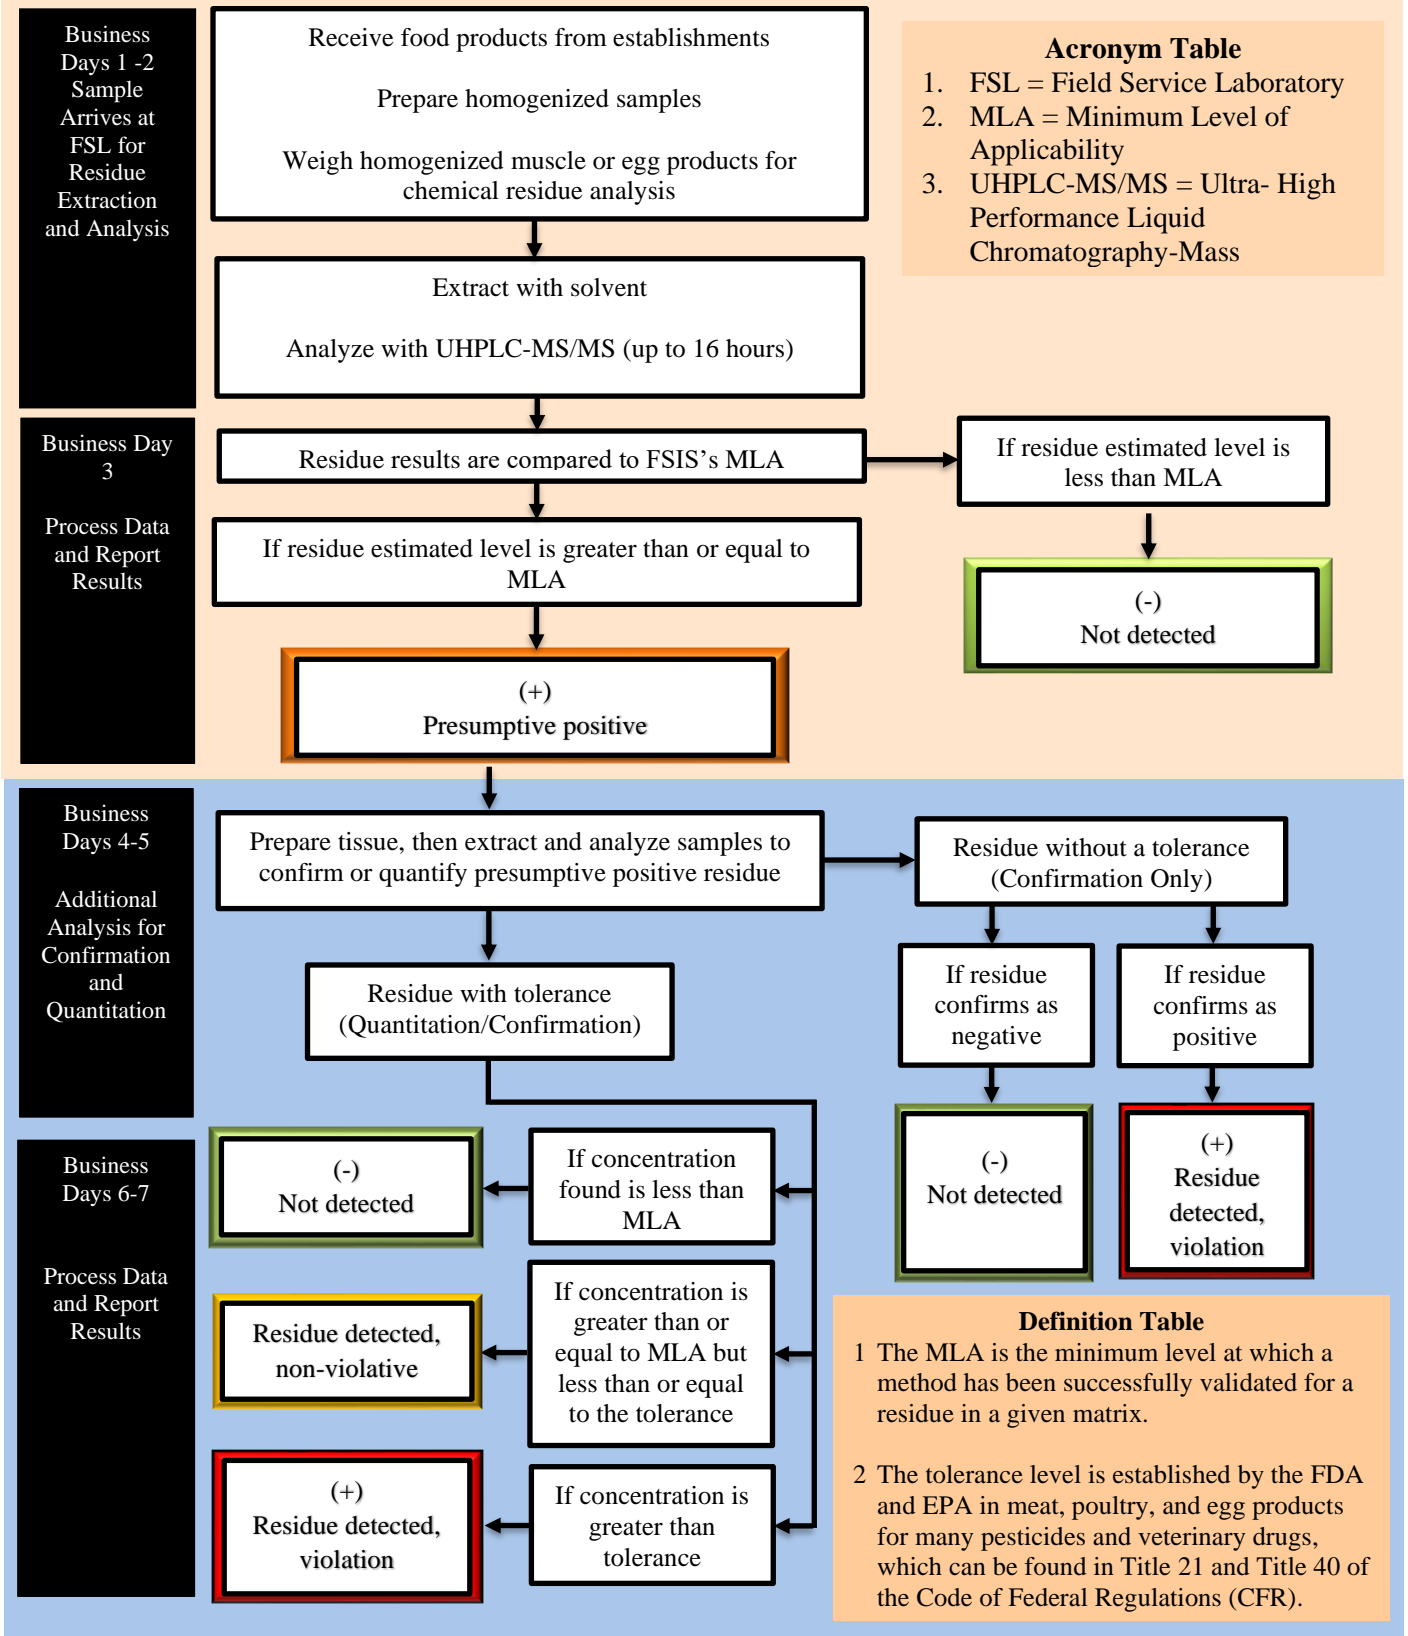

Blue background represents testing that exceeds the scope of this method. CLG-MEGA1 is a screening method and therefore, confirmation and quantitation analysis will be conducted with additional methods to determine if a sample is violative.

The Notice of Change for CLG-MEGA1 Appendix 1.00 is found in CLG-MEGA1.