



United States Department of Agriculture

Food Safety and Inspection Service
Office of Public Health Science
Laboratory Quality Assurance,
Response and Coordination Staff
950 College Station Rd.
Athens, GA 30605

Laboratory Guidebook Notice of Change


New, revised, or archived: CLG-MRQ1 Appendix 1.00

Title: Flow Chart Specific for FSIS Laboratory Quantitation of Animal Drug Residues
by HRAM LC-MS.

Effective Date: 09/29/23

Description and purpose of change: None

Flow Chart Specific for FSIS Laboratory Quantitation for Animal Drug Residues by HRAM LC-MS

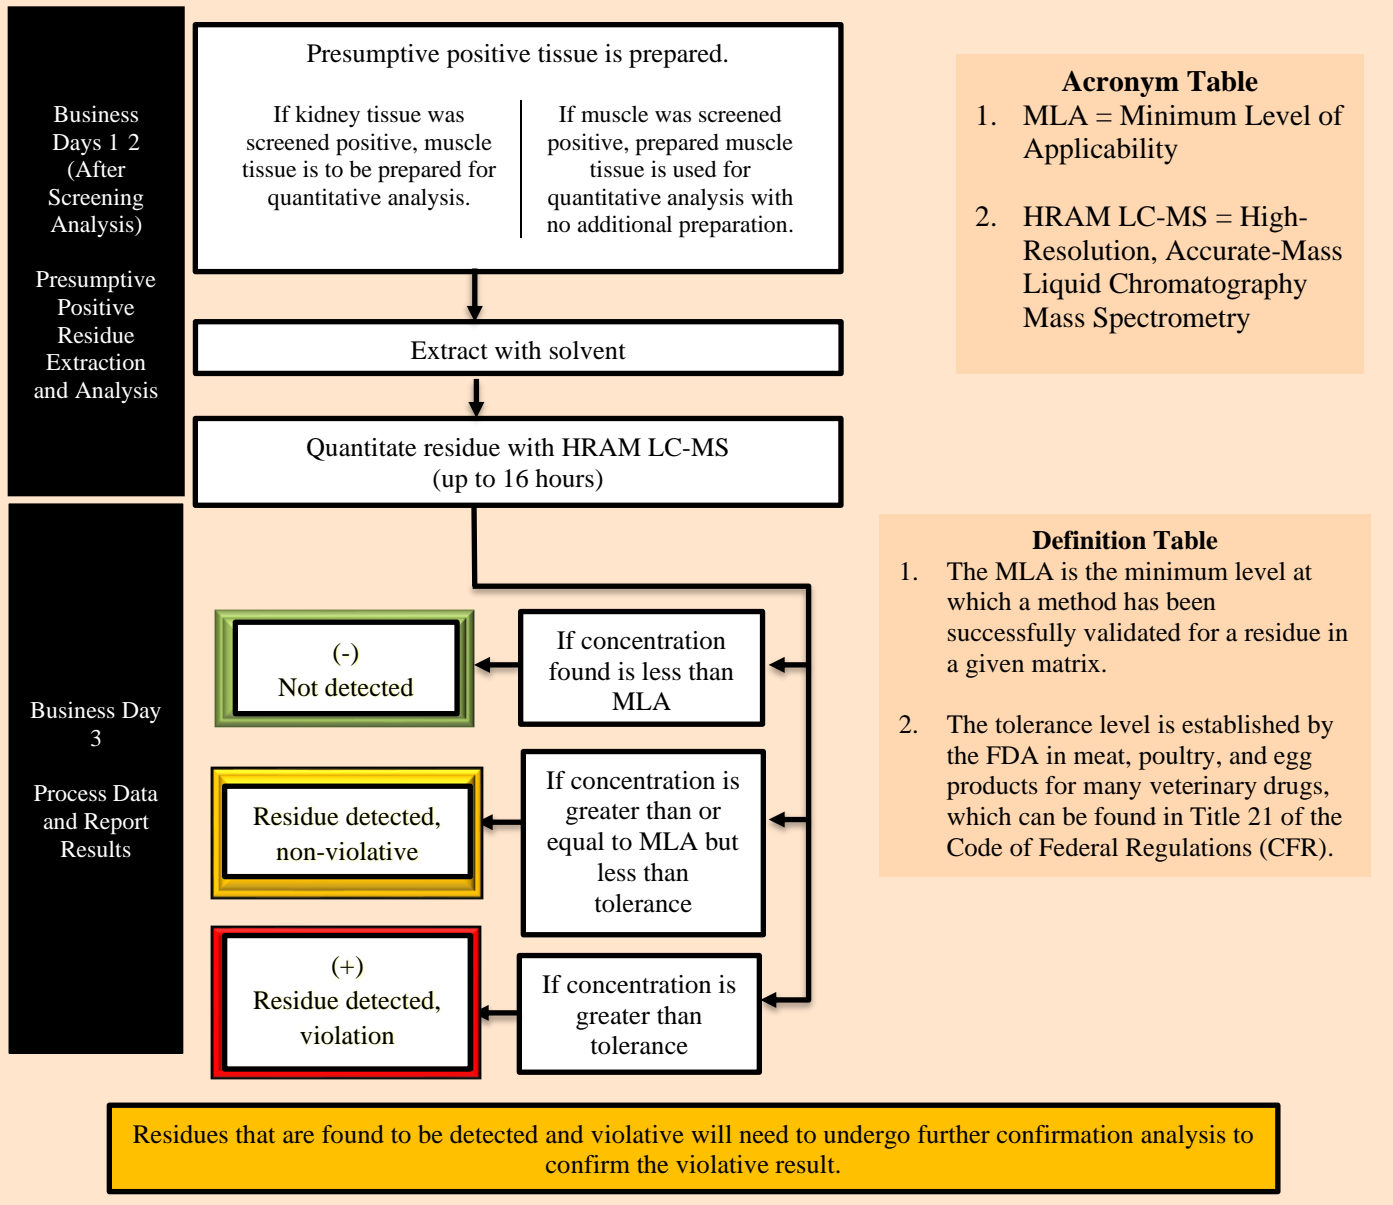

Acronym Table

1. MLA = Minimum Level of Applicability
2. HRAM LC-MS = High-Resolution, Accurate-Mass Liquid Chromatography Mass Spectrometry

Definition Table

1. The MLA is the minimum level at which a method has been successfully validated for a residue in a given matrix.
2. The tolerance level is established by the FDA in meat, poultry, and egg products for many veterinary drugs, which can be found in Title 21 of the Code of Federal Regulations (CFR).